



# Human Factor IX ELISA Kit

**Vertrieb:**

**L O X O GmbH** Immunbiologie Biochemie, Produkte und Systeme  
Postfach 11 30 69215 Dossenheim  
**Telefon** +49 (0) 62 21 - 86 80 23 **FAX** +49 (0) 62 21 - 86 80 255  
**E-Mail:** info@loxo.de **Internet:** www.loxo.de

Assaypro LLC  
30 Triad South Drive  
St. Charles, MO 63304  
T (636) 447-9175  
F (636) 447-9475  
[www.assaypro.com](http://www.assaypro.com)

**Hinweis/Note:**

Der Packungsbeileger dient nur als erste Information.  
Der relevante Packungsbeileger liegt der Ware bei.

The datasheet is only a first information.  
The relevant datasheet is included with the product.

For any questions regarding troubleshooting or performing the assay, please contact our support team at [support@assaypro.com](mailto:support@assaypro.com).


Thank you for choosing Assaypro.

## Assay Summary


Add 50  $\mu$ l of Standard/ Sample per well.  
Incubate 2 hours.




Wash, then add 50  $\mu$ l of  
Biotinylated Antibody per well.  
Incubate 1 hour.



Wash, then add 50  $\mu$ l of  
SP Conjugate per well.  
Incubate 30 minutes.



Wash, then add 50  $\mu$ l of  
Chromogen Substrate per well.  
Incubate 10 minutes.



Add 50  $\mu$ l of Stop Solution per well.  
Read at 450 nm immediately.





# AssayMax Human Factor IX ELISA Kit

Catalog No. EF1009-1  
Sample Insert/Reference Only

## Introduction

Factor IX (FIX) is a zymogen of plasma serine proteases required for normal hemostasis (1). FIX and FX are activated by tissue factor (TF) and factor VIIa (FVIIa) complexes and initiates coagulation resulting in thrombin formation (2). Hemophilia B is an X-linked bleeding disorder that results from a deficiency in functional coagulation factor IX (hFIX) (3). On the other hand, increased plasma level of FIX was reported to be an independent risk factor of venous thromboembolism (VTE) (4).

## Principle of the Assay

The AssayMax Human Factor IX ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for detection of human factor IX in plasma, serum, CSF, and cell culture supernatant samples. This assay employs a quantitative sandwich enzyme immunoassay technique that measures factor IX in less than 4 hours. A polyclonal antibody specific for factor IX has been pre-coated onto a 96-well microplate with removable strips. Factor IX in standards and samples is sandwiched by the immobilized antibody and the biotinylated polyclonal antibody specific for factor IX, which is recognized by a streptavidin-peroxidase conjugate. All unbound material is then washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

## Caution and Warning

- **Prepare all reagents (working diluent buffer, wash buffer, standards, biotinylated antibody, and SP conjugate) as instructed, prior to running the assay.**
- **Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this protocol. However, the user should determine the optimal dilution factor.**
- **Spin down the SP conjugate vial and the biotinylated antibody vial before opening and using contents.**
- This kit is for research use only.
- The kit should not be used beyond the expiration date.
- The Stop Solution is an acidic solution.

## Reagents

- **Human Factor IX Microplate:** A 96 well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against Factor IX.
- **Sealing Tapes:** Each kit contains 3 precut, pressure sensitive sealing tapes that can be cut to fit the format of the individual assay.
- **Human Factor IX Standard:** Human Factor IX in a buffered protein base (300 ng, lyophilized).
- **Biotinylated Human Factor IX Antibody (50x):** A 50-fold concentrated biotinylated polyclonal antibody against FIX (140  $\mu$ l).
- **EIA Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml, 2 bottles).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (80  $\mu$ l).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

## Storage Condition

- Upon arrival, immediately store components of the kit at recommended temperatures up to the expiration date.
- Store SP Conjugate and Biotinylated Antibody at -20°C.
- Store Microplate, Diluent Concentrate (10x), Wash Buffer, Stop Solution, and Chromogen Substrate at 2-8°C.
- Unused microplate wells may be returned to the foil pouch with the desiccant packs and resealed. May be stored for up to 30 days in a vacuum desiccator.
- Diluent (1x) may be stored for up to 30 days at 2-8°C.
- Store Standard at 2-8°C before reconstituting with diluent and at -20°C after reconstituting with diluent.

## Other Supplies required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20  $\mu$ l, 20-200  $\mu$ l, 200-1000  $\mu$ l, and multiple channel pipettes).
- Deionized or distilled reagent grade water.

## Sample Collection, Preparation and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 3000 x *g* for 10 minutes and collect supernatants. Dilute samples 1:400 into EIA Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles (EDTA or Heparin can also be used as an anticoagulant).
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 3000 x *g* for 10 minutes and remove serum. Dilute samples 1:400 into EIA Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles
- **Cell Culture Supernatants:** Collect cell culture media and centrifuge at 3000 x *g* for 10 minutes at 4°C to remove debris. Collect supernatants and assay. Samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **CSF:** Collect cerebrospinal fluid (CSF) using sample pot. Centrifuge samples at 3000 x *g* for 10 minutes and assay. Samples can be stored at -80°C for up to 3 months. Avoid repeated freeze-thaw cycles.

## Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use.
- **EIA Diluent Concentrate (10x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the EIA Diluent Concentrate 1:10 with reagent grade water. Store for up to 30 days at 2-8°C.
- **Human Factor IX Standard:** Reconstitute the 300 ng (60 mU) of Human Factor IX Standard with 3 ml of EIA Diluent to generate a 100 ng/ml (20 mU/ml) standard solution. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by serially diluting the standard solution (100 ng/ml) 1:2 with EIA Diluent to produce 50, 25, 12.5, 6.25, 3.125, and 1.563 ng/ml solutions. EIA Diluent serves as the zero standard (0 ng/ml). Any remaining solution should be frozen at -20°C and used within 30 days.

Standard Point	Dilution	[FIX] (ng/ml)	[FIX] (mU/ml)
P1	Standard (100 ng/ml)	100.0	20.00
P2	1 part P1 + 1 part EIA Diluent	50.00	10.00
P3	1 part P2 + 1 part EIA Diluent	25.00	5.000
P4	1 part P3 + 1 part EIA Diluent	12.50	2.500
P5	1 part P4 + 1 part EIA Diluent	6.250	1.250
P6	1 part P5 + 1 part EIA Diluent	3.125	0.625
P7	1 part P6 + 1 part EIA Diluent	1.563	0.313
P8	EIA Diluent	0.000	0.000

- **Biotinylated Human Factor IX Antibody (50x):** Spin down the antibody briefly and dilute the desired amount of the antibody 1:50 with EIA Diluent. Any remaining solution should be frozen at -20°C.
- **Wash Buffer Concentrate (20x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP Conjugate briefly and dilute the desired amount of the conjugate 1:100 with EIA Diluent. Any remaining solution should be frozen at -20°C.

### Assay Procedure

- Prepare all reagents, standard solutions, and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature (20-25°C).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccants inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 50 µl of Human Factor IX Standard or sample per well. Cover wells with a sealing tape and incubate for 2 hours. Start the timer after the last addition.
- Wash five times with 200 µl of Wash Buffer manually. Invert the plate each time and decant the contents; hit 4-5 times on absorbent material to completely remove the liquid. If using a machine, wash six times with 300 µl of Wash Buffer and then invert the plate, decanting the contents; hit 4-5 times on absorbent material to completely remove the liquid.
- Add 50 µl of Biotinylated Human Factor IX Antibody to each well and incubate for 1 hour.
- Wash the microplate as described above.
- Add 50 µl of Streptavidin-Peroxidase Conjugate per well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.



- Wash the microplate as described above.
- Add 50  $\mu$ l of Chromogen Substrate per well and incubate for about 10 minutes or till the optimal color density develops. Gently tap the plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50  $\mu$ l of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. If wavelength correction is available, subtract readings at 570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some unstable black particles may be generated at high concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.


### Data Analysis

- Calculate the mean value of the duplicate or triplicate for each standard and sample.
- To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.


### Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

f IX Standard Curve

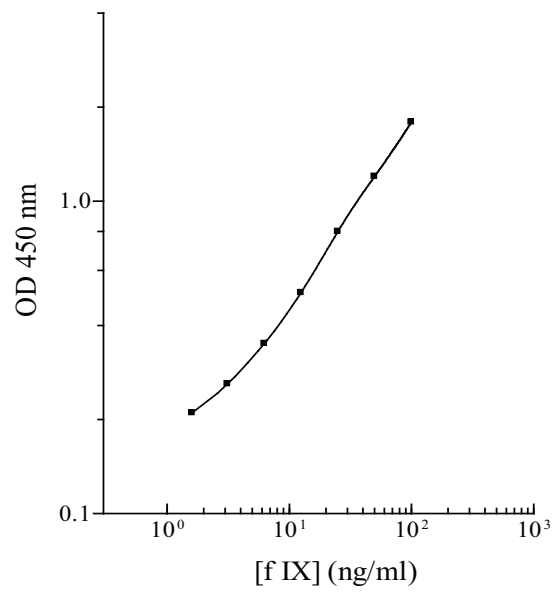

f IX Standard Curve

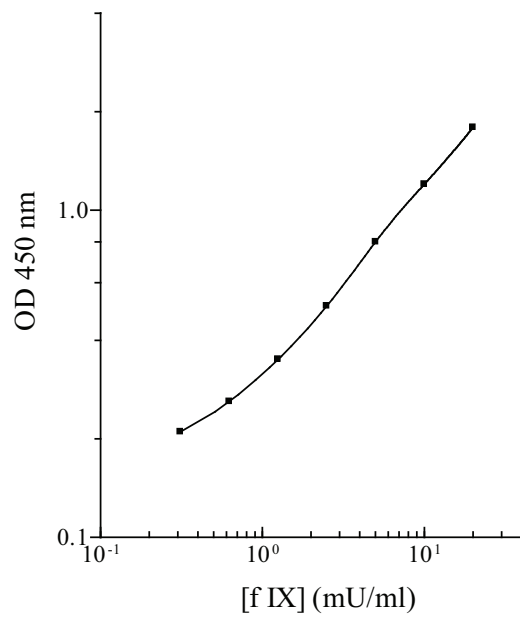

### Performance Characteristics

- The minimum detectable level of Factor IX was typically ~ 1.5 ng/ml.
- Intra-assay and inter-assay coefficients of variation were 5.0% and 7.1% respectively.
- **Kit standard has been calibrated against WHO International Standard.**

## Linearity

Sample Dilution	Average Percentage of Expected Value	
	Plasma	Serum
1:200	92%	91%
1:400	98%	99%
1:800	103%	104%

## Recovery

Standard Added Value	6.25 – 50 ng/ml
Recovery %	92 – 109%
Average Recovery %	97.5%

## Cross-Reactivity

Species	% Cross Reactivity
Beagle	None
Bovine	None
Monkey	<40%
Mouse	None
Rat	None
Swine	None
Rabbit	None
Proteins	% Cross Reactivity
Human Factor IX	100%
Human Factor IXa	100%

- 10% FBS in culture media will not affect the assay.

## Reference Value

- On average, normal human factor IX plasma level is 5 µg/ml.

## References

- (1) Wang X. *et al.* (2005) *J Thromb Haemost.* 3(4): 695-702
- (2) Bogdanov VY *et al* (2003) *Nat Med.* 9(4): 458-62
- (3) Pipe SW (2004) *Semin Thromb Hemost.* 30(2): 227-37
- (4) Bertina RM. (2003) *Pathophysiol Haemost Thromb.* 33(5-6): 395-400.

Version 7.6