

Human Fibronectin ELISA Kit

Vertrieb:

L O X O GmbH Immunbiologie Biochemie, Produkte und Systeme Postfach 11 30 69215 Dossenheim

Telefon +49 (0) 62 21 - 86 80 23 **FAX** +49 (0) 62 21 - 86 80 255

E-Mail: info@loxo.de **Internet:** www.loxo.de

Assaypro LLC 30 Triad South Drive St. Charles, MO 63304 T (636) 447-9175 F (636) 447-9475

www.assaypro.com

For any questions regarding troubleshooting or performing the assay, please contact our support team at support@assaypro.com.

Thank You for choosing Assaypro

Hinweis/Note:

Der Packungsbeileger dient nur als erste Information. Der relevante Packungsbeileger liegt der Ware bei.

The datasheet is only a first information. The relevant datasheet is included with the product.

Symbol Key



Consult instructions for use.

Assay Summary

Add 50 μl of Standard/ Sample per well. Incubate 2 hours.



Wash, then add 50 μl of Biotinylated Antibody per well. Incubate 1 hour.



Wash, then add 50 μl of SP Conjugate per well. Incubate 30 minutes.



Wash, then add 50 μl of Chromogen Substrate per well. Incubate 12 minutes.



Add 50 μl of Stop Solution per well. Read at 450 nm immediately.

Assay Template

12								
11								
10								
6								
∞								
7								
9								
5								
4								
æ								
2								
н								
	А	В	C	Q	ш	ш	ŋ	I

AssayMax Human Fibronectin ELISA Kit

Catalog No. EF2045-1 Sample Insert/Reference Only

Introduction

Fibronectin (FN) is a major component of the extracellular matrix and blood plasma and is a specific ligand for several integrin adhesion receptors (1). FN plays an important role not only in cell adhesion (2) and wound healing (3), but also in embryogenesis (4) and hematopoiesis (5). FN is over-expressed in cardiovascular disease states such as atherosclerosis (6) and myocardial infarction (7). Reduced levels of FN have been reported in patients with Disseminated Intravascular Coagulation (DIC) and low concentrations appear to correlate with a poor prognosis (8).

Principle of the Assay

The AssayMax Human Fibronectin ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for detection of human FN in milk, saliva, urine, CSF, and cell culture samples. This assay employs a quantitative sandwich enzyme immunoassay technique that measures human FN in less than 4 hours. A polyclonal antibody specific for human FN has been pre-coated onto a 96-well microplate with removable strips. FN in standards and samples is sandwiched by the immobilized polyclonal antibody and biotinylated polyclonal antibody specific for human FN, which is recognized by a streptavidin-peroxidase conjugate. All unbound material is then washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

Caution and Warning

- Prepare all reagents (working diluent buffer, wash buffer, standard, biotinylated antibody, and SP conjugate) as instructed, prior to running the assay.
- Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this protocol. However, the user should determine the optimal dilution factor.
- Spin down the SP conjugate vial and the biotinylated antibody vial before opening and using contents.
- This kit is for research use only.

- The kit should not be used beyond the expiration date.
- The Stop Solution is an acidic solution.

Reagents

- **Human FN Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against FN.
- **Sealing Tapes:** Each kit contains 3 precut, pressure sensitive sealing tapes that can be cut to fit the format of the individual assay.
- Human FN Standard: Human FN in a buffered protein base (1.5 μg, lyophilized).
- **Biotinylated Human FN Antibody (50x):** A 50-fold concentrated biotinylated polyclonal antibody against human FN (140 µl).
- MIX Diluent Concentrate (10x): A 10-fold concentrated buffered protein base (30 ml).
- Wash Buffer Concentrate (20x): A 20-fold concentrated buffered surfactant (30 ml, 2 bottles).
- Streptavidin-Peroxidase Conjugate (SP Conjugate): A 100-fold concentrate (80 μl).
- **Chromogen Substrate**: A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution**: A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

Storage Condition

- Upon arrival, immediately store components of the kit at recommended temperatures up to the expiration date.
- Store SP Conjugate and Biotinylated Antibody at -20°C.
- Store Microplate, Diluent Concentrate (10x), Wash Buffer, Stop Solution, and Chromogen Substrate at 2-8°C.
- Unused microplate wells may be returned to the foil pouch with the desiccant packs and resealed. May be stored for up to 30 days in a vacuum desiccator.
- Diluent (1x) may be stored for up to 30 days at 2-8°C.
- Store Standard at 2-8°C before reconstituting with Diluent and at -20°C after reconstituting with Diluent.

Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20 μl, 20-200 μl, 200-1000 μl, and multiple channel).
- Deionized or distilled reagent grade water.

Sample Collection, Preparation and Storage

- **Cell Culture Supernatants:** Centrifuge cell culture supernatants at 3000 x g for 10 minutes to remove debris. Collect supernatants and assay. Store samples at -20°C or below. Avoid repeated freeze-thaw cycles.
- **Urine:** Collect urine using sample pot. Centrifuge samples at 800 x g for 10 minutes. Dilute samples 1:2 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- Saliva: Collect saliva using sample tube. Centrifuge samples at 800 x g for 10 minutes. Dilute saliva 1:20 into MIX Diluent or within the range of 1:20 to 1:80, and assay. The user should determine the optimal dilution factor. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Milk:** Collect milk using sample tube. Centrifuge samples at 800 x g for 10 minutes. Milk dilution is suggested at 1:200 in MIX Diluent; however, the user should determine the optimal dilution factor. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **CSF:** Collect cerebrospinal fluid (CSF) using sample pot. Centrifuge samples at 3000 x g for 10 minutes. Dilute samples 1:100 into MIX Diluent and assay. The undiluted samples can be stored at -80°C for up to 3 months. Avoid repeated freeze-thaw cycles.

Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use.
- MIX Diluent Concentrate (10x): If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved.
 Dilute the MIX Diluent Concentrate 1:10 with reagent grade water. Store at 2-8°C and use within 30 days.
- Standard Curve: Reconstitute the 1.5 μ g of Human FN Standard with 1.5 ml of MIX Diluent to generate a 1 μ g/ml standard solution. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by serially diluting the standard solution (1 μ g/ml) 1:4 with MIX Diluent to produce 0.25, 0.063, 0.016, and 0.004 μ g/ml solutions. MIX Diluent serves as the zero standard (0 μ g/ml). Any remaining solution should be frozen at -20°C and used within 30 days.

Standard Point	Dilution	[FN] (μg/ml)
P1	Standard (1 μg/ml)	1.000
P2	1 part P1 + 3 parts MIX Diluent	0.250
Р3	1 part P2 + 3 parts MIX Diluent	0.063
P4	1 part P3 + 3 parts MIX Diluent	0.016
P5	1 part P4 + 3 parts MIX Diluent	0.004
P6	MIX Diluent	0.000

- **Biotinylated Human FN Antibody (50x):** Spin down the antibody briefly and dilute the desired amount of the antibody 1:50 with MIX Diluent. Any remaining solution should be frozen at -20°C.
- Wash Buffer Concentrate (20x): If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved.
 Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP conjugate briefly and dilute the desired amount of the conjugate 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.

Assay Procedure

- Prepare all reagents, standard solutions, and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature (20-25°C).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccants inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 50 μ l of Human Fibronectin Standard or sample per well. Cover wells with a sealing tape and incubate for 2 hours. Start the timer after the last addition.
- Wash five times with 200 µl of Wash Buffer manually. Invert the plate each time and decant the contents; hit 4-5 times on absorbent material to completely remove the liquid. If using a machine, wash six times with 300 µl of Wash Buffer and then invert the plate, decanting the contents; hit 4-5 times on absorbent material to completely remove the liquid.
- Add 50 μ l of Biotinylated Human FN antibody to each well and incubate for 1 hour.
- Wash the microplate as described above.
- Add 50 μ l of Streptavidin-Peroxidase conjugate to each well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash the microplate as described above.

- Add 50 μ l of Chromogen Substrate per well and incubate for 12 minutes or till the optimal blue color density develops. Gently tap plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 μ l of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm immediately. If wavelength correction is available, subtract readings at 570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some unstable black particles may be generated at high concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.


Data Analysis

- Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
- To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using four-parameter or log-log logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

Standard Curve

• The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.



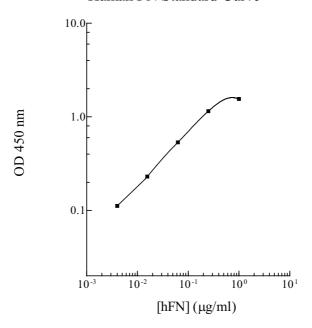

Performance Characteristics

- The minimum detectable dose of fibronectin is typically $\sim 0.004 \,\mu\text{g/ml}$.
- Intra-assay and inter-assay coefficients of variation were 4.9% and 7.0% respectively.

Linearity

	Average Percentage of Expected Value
Sample Dilution	Urine
No Dilution	91%
1:2	97%
1:4	106%

	Average Percentage of Expected Value
Sample Dilution	Milk
1:100	93%
1:200	98%
1:400	107%

	Average Percentage of Expected Value
Sample Dilution	Saliva
1:10	90%
1:20	97%
1:40	101%

Recovery

Standard Added Value	0.01 – 0.25 μg/ml	
Recovery %	89 – 113%	
Average Recovery %	97.5%	

Cross-Reactivity

Species	% Cross Reactivity
Monkey	<25%
Mouse	None
Rat	None
Swine	None
Canine	None
Bovine	None
Rabbit	None
Human	100%

References

- (1) Hynes, R.O. (1992) Cell 69:11
- (2) Wu, C. et al. (1995) Cell 83:715
- (3) Brown, L.F. et al. (1993) Am. J. Pathol. 142:793
- (4) Pagani, F. et al. (1991) J. Cell Biol. 113:1223
- (5) Verfaillie, C.M. et al. (1991) J. Exp. Med. 174:693
- (6) Glukhova M.A. et al. (1989) J. Cell. Biol. 109:357
- (7) Knowlton, A.A. et al. (1992) J. Clin. Invest. 89:1060
- (8) Cembrowski, G.S. and Mosherb, D.F. (1984) Thrombosis Research 36:437

Version 3.0

Related Products

- EF1045-1 AssayMax Human Fibronectin ELISA Kit (Plasma and Serum samples)
- EMF1045-1 AssayMax Mouse Fibronectin ELISA Kit (Plasma, Serum, Urine, and Cell Culture samples)
- ERF1045-1 AssayMax Rat Fibronectin ELISA Kit (Plasma, Serum, Urine, and Cell Culture samples)