



# Human Prealbumin ELISA Kit

**Vertrieb:**

**L O X O GmbH** Immunbiologie Biochemie, Produkte und Systeme  
Postfach 11 30 69215 Dossenheim  
**Telefon** +49 (0) 62 21 - 86 80 23 **FAX** +49 (0) 62 21 - 86 80 255  
**E-Mail:** info@loxo.de **Internet:** www.loxo.de

Assaypro LLC  
30 Triad South Drive  
St. Charles, MO 63304  
T (636) 447-9175  
F (636) 447-9475  
[www.assaypro.com](http://www.assaypro.com)

For any questions regarding troubleshooting or performing the assay, please contact our support team at [support@assaypro.com](mailto:support@assaypro.com).

Thank You for choosing Assaypro

**Hinweis/Note:**

Der Packungsbeileger dient nur als erste Information.  
Der relevante Packungsbeileger liegt der Ware bei.

The datasheet is only a first information.  
The relevant datasheet is included with the product.

## Assay Summary

**Step 1.** Add 50  $\mu$ l of Standard or Sample per well.  
Incubate 2 hours.

**Step 2.** Wash, then add 50  $\mu$ l of Biotinylated Antibody per well.  
Incubate 1 hour.

**Step 3.** Wash, then add 50  $\mu$ l of SP Conjugate per well.  
Incubate 30 minutes.

**Step 4.** Wash, then add 50  $\mu$ l of Chromogen Substrate per well.  
Incubate 25 minutes.

**Step 5.** Add 50  $\mu$ l of Stop Solution per well.  
Read at 450 nm immediately.

## Symbol Key



Consult instructions for use.





# AssayMax Human Prealbumin ELISA Kit

Catalog No. EP3010-1  
Sample Insert/Reference Only

## Introduction

Prealbumin (transthyretin) is a hepatic secretory protein thought to be important in the evaluation of nutritional deficiency and nutrition support (1). Prealbumin plays important physiological roles as a transporter of thyroxine and retinol-binding protein (2). Decreased prealbumin levels have been suggested to associate with malnutrition (3) and chronic kidney disease (4).

## Principle of the Assay

The AssayMax Human Prealbumin ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for detection of human prealbumin in **plasma, serum, urine, saliva, milk, CSF, and cell culture samples**. This assay employs a quantitative **sandwich enzyme immunoassay** technique that measures prealbumin in less than 4 hours. A polyclonal antibody specific for prealbumin has been pre-coated onto a 96-well microplate with removable strips. Prealbumin in standards and samples is sandwiched by the immobilized antibody and biotinylated polyclonal antibody specific for prealbumin, which is recognized by a streptavidin-peroxidase conjugate. All unbound material is washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

## Caution and Warning

- Prepare all reagents (working diluent buffer, wash buffer, standard, biotinylated antibody, and SP conjugate) as instructed, prior to running the assay.
- Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this protocol. However, the user should determine the optimal dilution factor.
- Spin down the SP conjugate vial and the biotinylated antibody vial before opening and using contents.
- This kit is for research use only.
- The kit should not be used beyond the expiration date.
- The Stop Solution is an acidic solution.

## Reagents

- **Human Prealbumin Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against human prealbumin.
- **Sealing Tapes:** Each kit contains 3 precut, pressure sensitive sealing tapes, which can be cut to fit the format of the individual assay.
- **Human Prealbumin Standard:** Human prealbumin in a buffered protein base (46.875 ng, lyophilized, 2 vials).
- **Biotinylated Human Prealbumin Antibody (100x):** A 100-fold concentrated biotinylated polyclonal antibody against prealbumin (80  $\mu$ l).
- **MIX Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml, 2 bottles).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (80  $\mu$ l).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

## Storage Condition

- Upon arrival, immediately store components of the kit at recommended temperatures up to the expiration date.
- Store SP Conjugate and Biotinylated Antibody at -20°C.
- Store Microplate, Diluent Concentrate (10x), Wash Buffer, Stop Solution, and Chromogen Substrate at 2-8°C.
- Unused microplate wells may be returned to the foil pouch with the desiccant packs and resealed. May be stored for up to 30 days in a vacuum desiccator.
- Diluent (1x) may be stored for up to 30 days at 2-8°C.
- Store Standard at 2-8°C before reconstituting with Diluent and at -20°C after reconstituting with Diluent.

## Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20  $\mu$ l, 20-200  $\mu$ l, 200-1000  $\mu$ l, and multiple channel).
- Deionized or distilled reagent grade water.

## Sample Collection and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 3000 x *g* for 10 minutes. Dilute samples 1:80000 into MIX Diluent or within the range of 1:40000 to 1:160000, and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles (EDTA or Heparin can also be used as an anticoagulant).
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 3000 x *g* for 10 minutes, and remove serum. Dilute samples 1:80000 into MIX Diluent or within the range of 1:40000 to 1:160000, and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Cell Culture Supernatants:** Centrifuge cell culture media at 3000 x *g* for 10 minutes to remove debris and collect supernatants. Dilute samples 1:10 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Urine:** Collect urine using sample pot. Centrifuge samples at 800 x *g* for 10 minutes and assay. Store samples at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Saliva:** Collect saliva using sample tube. Centrifuge samples at 800 x *g* for 10 minutes. Dilute samples 1:100 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Milk:** Collect milk using sample tube. Centrifuge samples at 800 x *g* for 10 minutes. Milk dilution is suggested at 1:1000 in MIX Diluent; however, the user should determine the optimal dilution factor. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **CSF:** Collect cerebrospinal fluid (CSF) using sample pot. Centrifuge samples at 3000 x *g* for 10 minutes. Dilute samples 1:4000 into MIX Diluent and assay. The undiluted samples can be stored at -80°C for up to 3 months. Avoid repeated freeze-thaw cycles.

***Refer to Sample Dilution Guidelines below for further instruction.***

Guidelines for Dilutions of 1:100 or Greater (for reference only; please follow the protocol for specific dilution suggested)	
<b>1:100</b>	<b>1:10000</b>
A) 4 $\mu$ l sample: 396 $\mu$ l buffer(100x) = 100 fold dilution  <i>Assuming the needed volume is less than or equal to 400 <math>\mu</math>l.</i>	A) 4 $\mu$ l sample : 396 $\mu$ l buffer (100x) B) 4 $\mu$ l of A : 396 $\mu$ l buffer (100x) = 10000 fold dilution  <i>Assuming the needed volume is less than or equal to 400 <math>\mu</math>l.</i>
<b>1:1000</b>	<b>1:100000</b>
A) 4 $\mu$ l sample : 396 $\mu$ l buffer (100x) B) 24 $\mu$ l of A : 216 $\mu$ l buffer (10x) = 1000 fold dilution  <i>Assuming the needed volume is less than or equal to 240 <math>\mu</math>l.</i>	A) 4 $\mu$ l sample : 396 $\mu$ l buffer (100x) B) 4 $\mu$ l of A : 396 $\mu$ l buffer (100x) C) 24 $\mu$ l of B : 216 $\mu$ l buffer (10x) = 100000 fold dilution  <i>Assuming the needed volume is less than or equal to 240 <math>\mu</math>l.</i>

## Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use.
- MIX Diluent Concentrate (10x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the MIX Diluent Concentrate 1:10 with reagent grade water. Store for up to 30 days at 2-8°C.
- Human Prealbumin Standard:** Reconstitute the 46.875 ng of Human Prealbumin Standard with 1.5 ml of MIX Diluent to generate a 31.25 ng/ml standard solution. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by further diluting the standard solution (31.25 ng/ml) 1:4 with MIX Diluent to produce 7.813, 1.953, 0.488, and 0.122 ng/ml solutions. MIX Diluent serves as the zero standard (0 ng/ml). **Any remaining solution should be frozen at -20°C and used within 3 days.**

Standard Point	Dilution	[Prealbumin] (ng/ml)
P1	Standard (31.25 ng/ml)	31.25
P2	1 part P1 + 3 parts MIX Diluent	7.813
P3	1 part P2 + 3 parts MIX Diluent	1.953
P4	1 part P3 + 3 parts MIX Diluent	0.488
P5	1 part P4 + 3 parts MIX Diluent	0.122
P6	MIX Diluent	0.000

- Biotinylated Human Prealbumin Antibody (100x):** Spin down the antibody briefly and dilute the desired amount of the antibody 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.



- **Wash Buffer Concentrate (20x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP conjugate briefly and dilute the desired amount of the conjugate 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.

## Assay Procedure

- Prepare all reagents, standard solutions, and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature (20-25°C).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccants inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 50 µl of Human Prealbumin Standard or sample per well. Cover wells with a sealing tape and incubate for 2 hours. Start the timer after the last addition.
- Wash five times with 200 µl of Wash Buffer manually. Invert the plate each time and decant the contents; hit 4-5 times on absorbent material to completely remove the liquid. If using a machine, wash six times with 300 µl of Wash Buffer and then invert the plate, decanting the contents; hit 4-5 times on absorbent material to completely remove the liquid.
- Add 50 µl of Biotinylated Human Prealbumin Antibody to each well and incubate for 1 hour.
- Wash the microplate as described above.
- Add 50 µl of Streptavidin-Peroxidase Conjugate per well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash the microplate as described above.
- Add 50 µl of Chromogen Substrate per well and incubate for 25 minutes or till the optimal blue color density develops. Gently tap plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 µl of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. If wavelength correction is available, subtract readings at 570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some unstable black particles may be generated at high concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.

## Data Analysis

- Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
- To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

## Typical Data


- The typical data is provided for reference only. Individual laboratory means may vary from the values listed. Variations between laboratories may be caused by technique differences.

Standard Point	ng/ml	OD	Average OD
P1	31.25	1.612 1.668	1.640
P2	7.813	1.270 1.174	1.222
P3	1.953	0.703 0.665	0.684
P4	0.488	0.298 0.301	0.300
P5	0.122	0.189 0.188	0.188
P6	0.000	0.121 0.134	0.127
<b>Sample: Pool Normal, Sodium Citrate Plasma (80000x)</b>		0.781 0.696	0.738

## Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

Human Prealbumin Standard Curve

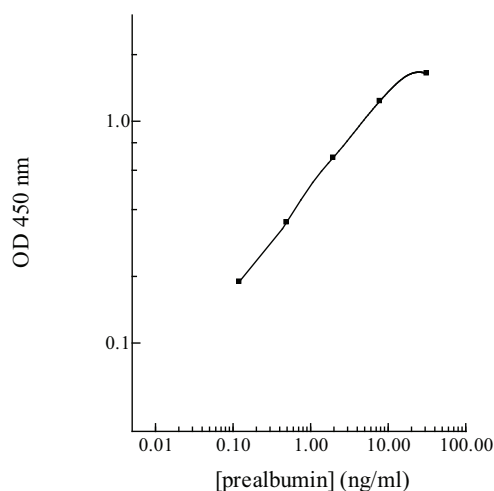

## Reference Value

- Normal human prealbumin plasma levels range from 120 to 450  $\mu\text{g/ml}$ .
- Human Plasma and Serum samples from healthy adults were tested (n=40). On average, prealbumin level was 231  $\mu\text{g/ml}$ .

Sample	n	Average Value ( $\mu\text{g/ml}$ )
Human Pool Normal Plasma	10	229
Human Normal Plasma	20	208
Human Pool Normal Serum	10	257

## Performance Characteristics

- The minimum detectable dose of prealbumin as calculated by 2SD from the mean of a zero standard was established to be 0.08 ng/ml.
- Intra-assay precision was determined by testing replicates of three plasma samples in one assay.
- Inter-assay precision was determined by testing three plasma samples in twenty assays.

Sample	Intra-Assay Precision			Inter-Assay Precision		
	1	2	3	1	2	3
n	20	20	20	20	20	20
CV (%)	4.4%	5.0%	4.1%	10.0%	9.1%	9.4%
Average CV (%)	4.5%			9.5%		

## Spiking Recovery

- Recovery was determined by spiking two plasma samples with different prealbumin concentrations.

Standard Added Value	0.5 – 5.0 ng/ml
Recovery %	88 – 113%
<b>Average Recovery %</b>	96%

## Linearity

- Plasma and serum samples were serially-diluted to test for linearity.

Sample Dilution	Average Percentage of Expected Value (%)	
	Plasma	Serum
1:40000	90%	91%
1:80000	98%	99%
1:160000	107%	106%

## Cross-Reactivity

Species	Cross Reactivity (%)
Canine	None
Monkey	None
Mouse	None
Rat	None
Swine	None
Rabbit	None
Bovine	None
Human	100%

## Troubleshooting

Issue	Causes	Course of Action
<b>Low Precision</b>	Use of expired components	<ul style="list-style-type: none"> <li>Check the expiration date listed before use.</li> <li>Do not interchange components from different lots.</li> </ul>
	Improper wash step	<ul style="list-style-type: none"> <li>Check that the correct wash buffer is being used.</li> <li>Check that all wells are dry after aspiration.</li> <li>Check that the microplate washer is dispensing properly.</li> <li>If washing by pipette, check for proper pipetting technique.</li> </ul>
	Splashing of reagents while loading wells	<ul style="list-style-type: none"> <li>Pipette properly in a controlled and careful manner.</li> </ul>
	Inconsistent volumes loaded into wells	<ul style="list-style-type: none"> <li>Pipette properly in a controlled and careful manner.</li> <li>Check pipette calibration.</li> <li>Check pipette for proper performance.</li> </ul>

	Insufficient mixing of reagent dilutions	<ul style="list-style-type: none"> <li>• Thoroughly agitate the Standard and Fluorescent Probe after reconstitution.</li> <li>• Thoroughly mix dilutions.</li> </ul>
	Improperly sealed microplate	<ul style="list-style-type: none"> <li>• Check the microplate pouch for proper sealing.</li> <li>• Check that the microplate pouch has no punctures.</li> <li>• Check that three desiccants are inside the microplate pouch prior to sealing.</li> </ul>
<b>Unexpectedly Low or High Signal Intensity</b>	Microplate was left unattended between steps	<ul style="list-style-type: none"> <li>• Each step of the procedure should be performed uninterrupted.</li> </ul>
	Omission of step	<ul style="list-style-type: none"> <li>• Consult the provided procedure for complete list of steps.</li> </ul>
	Steps performed in incorrect order	<ul style="list-style-type: none"> <li>• Consult the provided procedure for the correct order.</li> </ul>
	Insufficient amount of reagents added to wells	<ul style="list-style-type: none"> <li>• Check pipette calibration.</li> <li>• Check pipette for proper performance.</li> </ul>
	Wash step was skipped	<ul style="list-style-type: none"> <li>• Consult the provided procedure for all wash steps.</li> </ul>
	Improper wash buffer	<ul style="list-style-type: none"> <li>• Check that the correct wash buffer is being used.</li> </ul>
	Improper reagent preparation	<ul style="list-style-type: none"> <li>• Consult reagent preparation section for the correct dilutions of all reagents.</li> </ul>
	Insufficient or prolonged incubation periods	<ul style="list-style-type: none"> <li>• Consult the provided procedure for correct incubation time.</li> </ul>
<b>Deficient Standard Curve Fit</b>	Non-optimal sample dilution	<ul style="list-style-type: none"> <li>• Sandwich ELISA: If samples generate OD values higher than the highest standard point (P1), dilute samples further and repeat the assay.</li> <li>• Competitive ELISA: If samples generate OD values lower than the highest standard point (P1), dilute samples further and repeat the assay.</li> <li>• User should determine the optimal dilution factor for samples.</li> </ul>
	Contamination of reagents	<ul style="list-style-type: none"> <li>• A new tip must be used for each addition of different samples or reagents during the assay procedure.</li> </ul>
	Contents of wells evaporate	<ul style="list-style-type: none"> <li>• Verify that the aluminum sealing film is firmly in place before placing the assay in the incubator.</li> </ul>
	Improper pipetting	<ul style="list-style-type: none"> <li>• Pipette properly in a controlled and careful manner.</li> <li>• Check pipette calibration.</li> <li>• Check pipette for proper performance.</li> </ul>
		Insufficient mixing of reagent dilutions

## References

- (1) Chertow GM *et al.* (2005) *Kidney Int.* 68(6): 2794-800
- (2) Hamilton JA. *et al.*(2001) *Cell Mol Life Sci.* 58(10):1491-521
- (3) Beck FK. *et al.* (2002) *Am Fam Physician.* 15; 65(8): 1575-8
- (4) Kaysen GA. *et al.* (2004) *J Am Soc Nephrol*15 (3): 538-48

Version 7.0