



Human ApoH ELISA Kit

Vertrieb:

L O X O GmbH Immunbiologie Biochemie, Produkte und Systeme
Postfach 11 30 69215 Dossenheim
Telefon +49 (0) 62 21 - 86 80 23 **FAX** +49 (0) 62 21 - 86 80 255
E-Mail: info@loxo.de **Internet:** www.loxo.de

Assaypro LLC
30 Triad South Drive
St. Charles, MO 63304
T (636) 447-9175
F (636) 447-9475
www.assaypro.com

Hinweis/Note:

Der Packungsbeileger dient nur als erste Information.
Der relevante Packungsbeileger liegt der Ware bei.


The datasheet is only a first information.
The relevant datasheet is included with the product.

For any questions regarding troubleshooting or performing the assay, please contact our support team at support@assaypro.com.


Thank you for choosing Assaypro.

Assay Summary


Add 50 μ l of standard/sample per well.
Incubate 2 hours.




Wash, then add 50 μ l of
biotinylated antibody per well.
Incubate 1 hour.



Wash, then add 50 μ l of SP per well.
Incubate 30 minutes.



Wash, then add 50 μ l of
Chromogen Substrate per well.
Incubate 10 minutes.



Add 50 μ l of Stop Solution per well.
Read at 450 nm immediately.

AssayMax Human Apolipoprotein H ELISA Kit

Catalog No. EA8821-1
Sample Insert/Reference Only

Introduction

Apolipoprotein H (ApoH), previously known as β_2 -glycoprotein I, is a 50 kDa plasma glycoprotein with 326 amino acids and circulates in plasma at about 200 $\mu\text{g}/\text{ml}$ (1-4). ApoH inhibits the generation of factor Xa, Xia, and Xlla, preventing activation of the intrinsic blood coagulation cascade (5, 6). Binding of ApoH to anionic phospholipids such as phosphatidylserine and cardiolipin plays a key role in the formation of antiphospholipid antibodies, involving in autoimmune diseases like antiphospholipid syndrome or systemic lupus erythematosus (7, 8). ApoH is increased in the plasma and liver of type 2 diabetic patients with metabolic syndrome and could be considered as a clinical marker of cardiovascular risk (9). ApoH interacts with viral proteins, such as the hepatitis B virus antigen, immunodeficiency virus type 1 and type 2 proteins, and Andes virus (10, 11).

Principle of the Assay

The AssayMax Human Apolipoprotein H ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for detection of human ApoH in plasma, serum, urine, saliva, milk, and cell culture samples. This assay employs a quantitative sandwich enzyme immunoassay technique that measures ApoH in less than 4 hours. A polyclonal antibody specific for human ApoH has been pre-coated onto a 96-well microplate with removable strips. ApoH in standards and samples is sandwiched by the immobilized antibody and biotinylated polyclonal antibody specific for ApoH, which is recognized by a streptavidin-peroxidase conjugate. All unbound material is then washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

Caution and Warning

- **Prepare all reagents (working diluent buffer, wash buffer, standards, biotinylated antibody, and SP conjugate) as instructed, prior to running the assay.**

- **Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this protocol. However, the user should determine the optimal dilution factor.**
- **Spin down the SP conjugate vial and the biotinylated antibody vial before opening and using contents.**
- This kit is for research use only.
- The kit should not be used beyond the expiration date.
- The Stop Solution is an acidic solution.

Reagents

- **Human ApoH Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against human ApoH.
- **Sealing Tapes:** Each kit contains 3 precut, pressure sensitive sealing tapes that can be cut to fit the format of the individual assay.
- **Human ApoH Standard:** Human ApoH in a buffered protein base (320 ng, lyophilized).
- **Biotinylated Human ApoH Antibody (100x):** A 100-fold concentrated biotinylated polyclonal antibody against ApoH (80 μ l).
- **MIX Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml, 2 bottles).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (80 μ l).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

Storage Condition

- Store components of the kit at 2-8°C or -20°C upon arrival up to the expiration date.
- Store SP Conjugate and biotinylated antibody at -20°C.
- Store Microplate, Diluent Concentrate (10x), Wash Buffer, Stop Solution, and Chromogen Substrate at 2-8°C.
- Unused microplate wells may be returned to the foil pouch with the desiccant packs and resealed. May be stored for up to 30 days in a vacuum desiccator.
- Diluent (1x) may be stored for up to 30 days at 2-8°C.
- Store standard at 2-8°C before reconstituting with diluent and at -20°C after reconstituting with diluent.

Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20 μ l, 20-200 μ l, 200-1000 μ l and multiple channel).
- Deionized or distilled reagent grade water.

Sample Collection, Preparation and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 3000 x *g* for 10 minutes. Dilute samples 1:20000 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles (EDTA or Heparin can also be used as an anticoagulant).
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 3000 x *g* for 10 minutes. Dilute samples 1:20000 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Cell Culture Media:** Centrifuge cell culture media at 3000 x *g* for 10 minutes to remove debris. Collect supernatants and assay. Store samples at -20°C or below. Avoid repeated freeze-thaw cycles.
- **Cell Lysate:** Rinse cell with cold PBS and then scrape the cell into a tube with 5 ml cold PBS with 0.5 M EDTA. Centrifuge suspension at 1500 rpm for 10 minutes at 4°C and aspirate supernatant. Re-suspend pellet in ice-cold Lysis Buffer (10 mM Tris, pH8.0, 130 mM NaCl, 1% Triton X-100, protease inhibitor cocktail). For every 1×10^6 cells add approximately 100 μ L of ice-cold Lysis Buffer. Incubate on ice for 60 minutes. Centrifuge at 13000 rpm for 30 minutes at 4°C and collect supernatant for assay.
- **Urine:** Collect urine using sample pot. Centrifuge sample at 800 x *g* for 10 minutes. Dilute sample 1:16 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Saliva:** Collect saliva using sample tube. Centrifuge sample at 800 x *g* for 10 minutes. Dilute sample 1:16 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Milk:** Collect milk using sample tube. Centrifuge sample at 800 x *g* for 10 minutes. Dilute sample 1:400 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use.
- **MIX Diluent Concentrate (10x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the MIX Diluent Concentrate 1:10 with reagent grade water. Store for up to 30 days at 2-8°C.
- **Standard Curve:** Reconstitute the 320 ng of Human ApoH Standard with 4 ml of MIX Diluent to generate a solution of 80 ng/ml. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by serially diluting the standard solution (80 ng/ml) 1:2 with MIX Diluent to produce 40, 20, 10, 5, 2.5, 1.25, and 0.625 ng/ml solutions. MIX Diluent serves as the zero standard (0 ng/ml). Any remaining solution should be frozen at -20°C and used within 30 days.

Standard Point	Dilution	[ApoH] (ng/ml)
P1	1 part Standard (80 ng/ml) + 1 part MIX Diluent	40.00
P2	1 part P1 + 1 part MIX Diluent	20.00
P3	1 part P2 + 1 part MIX Diluent	10.00
P4	1 part P3 + 1 part MIX Diluent	5.000
P5	1 part P4 + 1 part MIX Diluent	2.500
P6	1 part P5 + 1 part MIX Diluent	1.250
P7	1 part P6 + 1 part MIX Diluent	0.625
P8	MIX Diluent	0.000

- **Biotinylated Human ApoH Antibody (100x):** Spin down the antibody briefly and dilute the desired amount of the antibody 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.
- **Wash Buffer Concentrate (20x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP Conjugate briefly and dilute the desired amount of the conjugate 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.

Assay Procedure

- Prepare all reagents, working standards and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature (20-30°C).


- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccants inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 50 μ l of Human ApoH Standard or sample per well. Cover wells with a sealing tape and incubate for 2 hours. Start the timer after the last sample addition.
- Wash five times with 200 μ l of Wash Buffer manually. Invert the plate each time and decant the contents; hit 4-5 times on absorbent material to completely remove the liquid. If using a machine, wash six times with 300 μ l of Wash Buffer and then invert the plate, decanting the contents; hit 4-5 times on absorbent material to completely remove the liquid.
- Add 50 μ l of Biotinylated Human ApoH Antibody to each well and incubate for 1 hour.
- Wash the microplate as described above.
- Add 50 μ l of Streptavidin-Peroxidase Conjugate to each well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash the microplate as described above.
- Add 50 μ l of Chromogen Substrate per well and incubate for about 10 minutes or till the optimal blue color density develops. Gently tap plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 μ l of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. If wavelength correction is available, subtract readings at 570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some unstable black particles may be generated at high concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.

Data Analysis

- Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
- To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

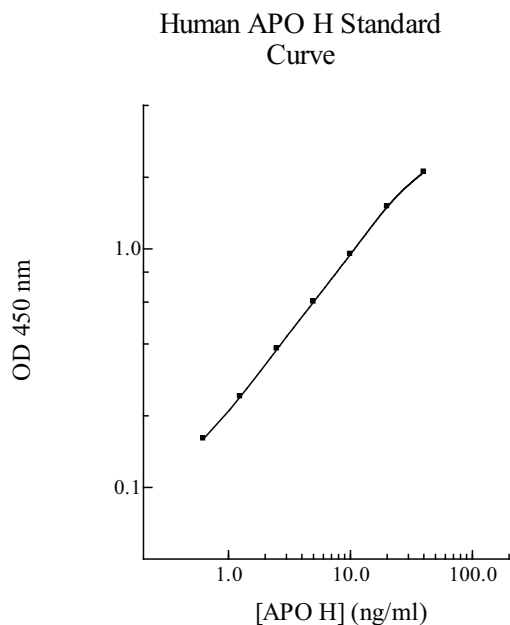

Performance Characteristics

- The minimum detectable dose of ApoH is typically ~ 0.6 ng/ml.
- Intra-assay and inter-assay coefficients of variation were 4.8 % and 7.2 % respectively.

Linearity

Sample Dilution	Average Percentage of Expected Value	
	Plasma	Serum
1:10000	91%	94%
1:20000	99%	100%
1:40000	104%	105%

Sample Dilution	Average Percentage of Expected Value	
	Urine	Saliva
1:8	90%	88%
1:16	100%	98%
1:32	105%	106%

Recovery

Standard Added Value	1 – 10 ng/ml
Recovery %	88% - 111%
Average Recovery %	98%

Cross-Reactivity

Species	% Cross Reactivity
Beagle	None
Bovine	None
Monkey	<50%
Mouse	None
Rat	None
Rabbit	None
Swine	<10%

- No significant cross reactivity observed with ApoA-I, ApoA-II, ApoB, ApoC-I, ApoC-II, and ApoC-III.

Reference Values

- Normal human ApoH plasma levels range from 200 to 400 µg/ml.

References

- (1) Lozier J. *et al.* (1984) Proc. Natl. Acad. Sci. U.S.A. 81:3640–3644
- (2) Steinkasserer A *et al.* (1991) Biochem. J. 277:387–391
- (3) Kristensen T *et al.* (1991) FEBS Lett. 289:183–186
- (4) Polz E and Lostner GM (1979) FEBS Lett. 102:183-186
- (5) Shi W *et al.* (1993) Thromb. Haemost. 70: 342–345
- (6) Schousboe I and Rasmussen MS (1995) Thromb. Haemost. 73: 798–804
- (7) McNeil HP *et al.* (1990) Proc. Natl. Acad. Sci. U.S.A. 87: 4120–4124
- (8) Timothy A *et al.* (1999) Biochem. J. 340:59-67
- (9) Castro A *et al.* (2010) Atherosclerosis 209:201-205
- (10) Stefas E *et al.* (1997) AIDS Res Hum Retroviruses 13:97-104
- (11) Godoy P *et al.* (2009) J. Virol. 83:5046-5055

Version 2.7