



Human Lactoferrin Autoantibody ELISA Kit (Anti-Lactoferrin IgG)

Vertrieb:

L O X O GmbH Immunbiologie Biochemie, Produkte und Systeme
Postfach 11 30 69215 Dossenheim
Telefon +49 (0) 62 21 - 86 80 23 **FAX** +49 (0) 62 21 - 86 80 255
E-Mail: info@loxo.de **Internet:** www.loxo.de

Assaypro LLC
3400 Harry S Truman Blvd
St. Charles, MO 63301
T (636) 447-9175
F (636) 395-7419
www.assaypro.com

Hinweis/Note:

Der Packungsbeileger dient nur als erste Information.
Der relevante Packungsbeileger liegt der Ware bei.

The datasheet is only a first information.
The relevant datasheet is included with the product.

For any questions regarding troubleshooting or performing the assay, please contact our support team at support@assaypro.com.

Thank you for choosing Assaypro.

Assay Summary

Step 1. Add 50 μ l of Standard or Sample per well.
Incubate 2 hours.

Step 2. Wash, then add 50 μ l of HRP Conjugate per well.
Incubate 1 hour.

Step 3. Wash, then add 50 μ l of Chromogen Substrate per well.
Incubate 30 minutes.

Step 4. Add 50 μ l of Stop Solution per well.
Read at 450 nm immediately.

Symbol Key



Consult instructions for use.

AssayMax Human Lactoferrin Autoantibody ELISA Kit (Anti-Lactoferrin IgG)

Catalog No. EL7011-1

Sample protocol for reference use only

Introduction

Lactoferrin is an 80 kDa iron-binding glycoprotein produced by many exocrine glands with a major constituent in the secondary granules of neutrophilic leukocytes. Serum lactoferrin concentration is much higher during inflammation (1). Lactoferrin is known to be an immune modulator or enhancer due to specific receptors for lactoferrin that are found on many key immune cells such as lymphocytes, monocytes, and macrophages. Lactoferrin is known to be directly involved in the up-regulation of natural killer (NK) cell activity (2). Lactoferrin is present in maternal milk, saliva, tears, vaginal secretions, semen, bronchoalveolar lavage fluid, and specific granules of polymorphonuclear leukocytes (PMNs) (3). Lactoferrin is found mainly in the oral cavity where it can come into direct contact with pathogens such as viruses, bacteria, etc. Lactoferrin directly inhibits viruses by binding to viral receptor sites, thus preventing the virus from infecting healthy cells. Lactoferrin has a direct bactericidal function to certain bacteria such as *Streptococcus mutans*, *Vibrio cholerae*, *Escherichia coli*, *Actinobacillus actinomycetemcomitans*, and *Legionella pneumophila* (2-4). Also, it has a bacteriostatic effect that deprives iron-requiring bacteria of this essential growth nutrient (4). Lactoferrin is also considered an antioxidant that scavenges free iron, helping to prevent uncontrolled iron based free radical reactions, thus protecting certain cells from peroxidation (2). Autoantibodies against lactoferrin belong to the pANCA class (Perinuclear Anti-Neutrophil Cytoplasmic Antibodies). Anti-lactoferrin antibodies are found in patients with rheumatoid arthritis with vasculitis (5) as well as in reactive arthritis and ankylosing spondylitis (6).

Principle of the Assay

The AssayMax Human Lactoferrin Autoantibody ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for the quantitative determination of autoimmune response (IgG) to a target antigen (lactoferrin). The kit detects autoantibodies in **plasma and serum samples**. This assay employs a quantitative **sandwich enzyme immunoassay technique that measures autoantibodies (anti-Lactoferrin IgG) in less than 4 hours**. A lactoferrin antigen has been pre-coated onto a 96-well microplate with removable strips. Autoantibody specific for lactoferrin in standards and samples is sandwiched

by the immobilized antigen and an antibody-HRP conjugate. All unbound material is washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

Caution and Warning

- Prepare all reagents (working diluent buffer, wash buffer, standard, HRP conjugate) as instructed, prior to running the assay.
- Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this protocol. However, the user should determine the optimal dilution factor.
- Spin down the HRP conjugate vial before opening and using contents.
- The Stop Solution is an acidic solution.
- This kit is for research use only.
- The kit should not be used beyond the expiration date.

Reagents

- **Human Lactoferrin Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with lactoferrin.
- **Sealing Tapes:** Each kit contains 3 pre-cut, pressure sensitive sealing tapes that can be cut to fit the format of the individual assay.
- **Human Lactoferrin Standard:** Plasma standard (100 AU, lyophilized).
- **HRP Conjugate (50x):** A 50-fold concentrated HRP-antibody conjugate (120 μ l).
- **MIX Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml, 1 bottle).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

Storage Condition

- Upon arrival, immediately store components of the kit at recommended temperatures up to the expiration date.
- Store HRP Conjugate at -20°C.
- Store Microplate, Diluent Concentrate (10x), Wash Buffer, Stop Solution, and Chromogen Substrate at 2-8°C.
- Unused microplate wells may be returned to the foil pouch with the desiccant packs and resealed. May be stored for up to 30 days in a vacuum desiccator.

- Diluent (1x) may be stored for up to 30 days at 2-8°C.
- Store Standard at 2-8°C before reconstituting with Diluent and at -20°C after reconstituting with Diluent.

Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20 µl, 20-200 µl, 200-1000 µl, and multiple channel).
- Deionized or distilled reagent grade water.

Sample Collection, Preparation, and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 3000 x *g* for 10 minutes. Dilute samples 1:40 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles (EDTA or Heparin can also be used as an anticoagulant).
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 3000 x *g* for 10 minutes, and remove serum. Dilute samples 1:40 into MIX Diluent and assay. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use.
- **MIX Diluent Concentrate (10x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the MIX Diluent Concentrate 1:10 with reagent grade water. Store for up to 30 days at 2-8°C.
- **Standard Curve:** Reconstitute the Standard 100 AU with 1 ml of MIX Diluent to generate a 100 AU/ml standard stock solution. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate points by serially diluting the standard stock solution (100 AU/ml) 1:2 using equal volume of MIX Diluent to produce 50, 25, 12.5, 6.25, 3.125, and 1.563 AU/ml solutions. MIX Diluent serves as the zero standard (0 AU/ml). Any remaining solution should be frozen at -20°C and used within 30 days.

Standard Point	Dilution	[Lactoferrin] (AU/ml)
P1	1 part Standard (100 AU/ml)	100.0
P2	1 part P1 + 1 part MIX Diluent	50.00
P3	1 part P2 + 1 part MIX Diluent	25.00
P4	1 part P3 + 1 part MIX Diluent	12.50
P5	1 part P4 + 1 part MIX Diluent	6.250
P6	1 part P5 + 1 part MIX Diluent	3.125
P7	1 part P6 + 1 part MIX Diluent	1.563
P8	MIX Diluent	0.000

- **HRP Conjugate (50x):** Spin down the HRP Conjugate briefly and dilute the desired amount of the conjugate 1:50 with MIX Diluent. Any remaining solution should be frozen at -20°C.
- **Wash Buffer Concentrate (20x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.

Assay Procedure

- Prepare all reagents, standard solutions, and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature (20-25°C).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccants inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 50 µl of Standard or sample per well. Cover wells with a sealing tape and incubate for 2 hours. Start the timer after the last addition.
- Wash five times with 200 µl of Wash Buffer manually. Invert the plate each time and decant the contents; hit 4-5 times on absorbent material to completely remove the liquid. If using a machine, wash six times with 300 µl of Wash Buffer and then invert the plate, decanting the contents; hit 4-5 times on absorbent material to completely remove the liquid.
- Add 50 µl of HRP Conjugate to each well and incubate for 1 hour.
- Wash the microplate as described above.
- Add 50 µl of Chromogen Substrate per well and incubate for 30 minutes or till the optimal blue color density develops. Gently tap the plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 µl of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. If wavelength correction is available, subtract readings at

570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some unstable black particles may be generated at high concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.

Data Analysis

- Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
- To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve.
- Although normal samples have been diluted 1:40, do not multiply the value by the dilution factor. Samples with elevated level of autoantibodies can be diluted further; for example 1:80. Account for this further dilution factor when calculating the value of the sample.

Example	Dilution Factor	Multiplication Factor For Calculating Values
Serum with normal level of anti-Lactoferrin IgG	40x	1
Serum with elevated level of anti-Lactoferrin IgG	80x	2
Serum with elevated level of anti-Lactoferrin IgG	160x	4


Typical Data

- The typical data is provided for reference only. Individual laboratory means may vary from the values listed. Variations between laboratories may be caused by technique differences.

Standard Point	AU/ml	Average OD
P1	100.0	2.507
P2	50.00	1.932
P3	25.00	1.007
P4	12.50	0.543
P5	6.250	0.273
P6	3.125	0.166
P7	1.563	0.125
P8	0.000	0.055
Normal Level Sample (40x): Serum with normal level of anti-Lactoferrin IgG		0.301
Elevated Level Sample (80x): Serum with elevated level of anti-Lactoferrin IgG		0.624

Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

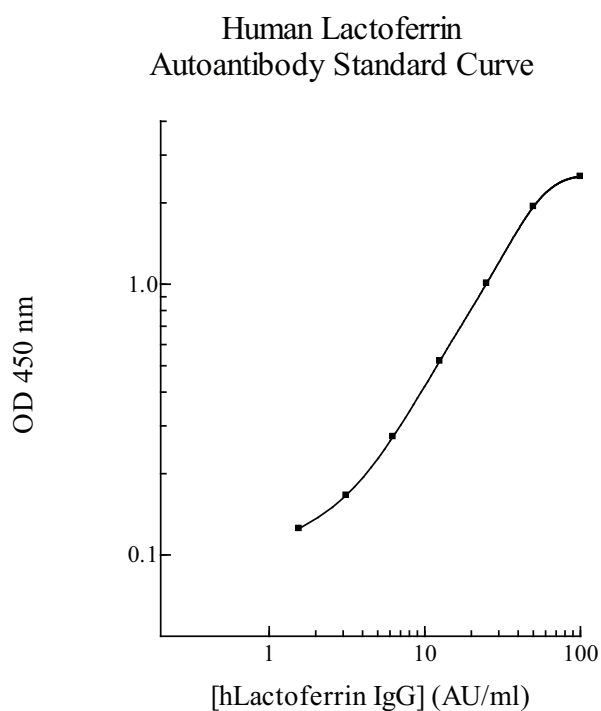

Reference Value

- Human plasma and serum samples from healthy adults were tested (n=20). Moreover, patient serum samples containing high levels of anti-lactoferrin IgG were tested (n=11). The following ranges have been established:

Sample	Anti-Lactoferrin IgG (AU/mL)
Normal Level	< 12.0
Elevated Level	≥ 12.0

- It is recommended that each laboratory establishes its own normal and pathological ranges of antibodies.

Performance Characteristics

- The minimum detectable dose of autoantibodies as calculated by 2SD from the mean of a zero standard was established to be 1 AU/ml.
- Intra-assay precision was determined by testing replicates of three plasma samples in one assay.
- Inter-assay precision was determined by testing three plasma samples in twenty assays.

	Intra-Assay Precision			Inter-Assay Precision		
Sample	1	2	3	1	2	3
n	20	20	20	20	20	20
CV (%)	4.0%	4.3%	5.1%	9.1%	8.9%	9.5%
Average CV (%)	4.5%			9.2%		

Linearity

- Serum samples were serially-diluted to test for linearity.

Average Percentage of Expected Value (%)	
Sample Dilution	Serum
1:20	90%
1:40	98%
1:80	105%

Troubleshooting

Issue	Causes	Course of Action
Low Precision	Use of expired components	<ul style="list-style-type: none"> • Check the expiration date listed before use. • Do not interchange components from different lots.
	Improper wash step	<ul style="list-style-type: none"> • Check that the correct wash buffer is being used. • Check that all wells are dry after aspiration. • Check that the microplate washer is dispensing properly. • If washing by pipette, check for proper pipetting technique.
	Splashing of reagents while loading wells	<ul style="list-style-type: none"> • Pipette properly in a controlled and careful manner.
	Inconsistent volumes loaded into wells	<ul style="list-style-type: none"> • Pipette properly in a controlled and careful manner. • Check pipette calibration. • Check pipette for proper performance.
	Insufficient mixing of reagent dilutions	<ul style="list-style-type: none"> • Thoroughly agitate the lyophilized components after reconstitution. • Thoroughly mix dilutions.
	Improperly sealed microplate	<ul style="list-style-type: none"> • Check the microplate pouch for proper sealing. • Check that the microplate pouch has no punctures. • Check that three desiccants are inside the microplate pouch prior to sealing.
Unexpectedly Low or High Signal Intensity	Microplate was left unattended between steps	<ul style="list-style-type: none"> • Each step of the procedure should be performed uninterrupted.
	Omission of step	<ul style="list-style-type: none"> • Consult the provided procedure for complete list of steps.
	Steps performed in incorrect order	<ul style="list-style-type: none"> • Consult the provided procedure for the correct order.
	Insufficient amount of reagents added to wells	<ul style="list-style-type: none"> • Check pipette calibration. • Check pipette for proper performance.
	Wash step was skipped	<ul style="list-style-type: none"> • Consult the provided procedure for all wash steps.
	Improper wash buffer	<ul style="list-style-type: none"> • Check that the correct wash buffer is being used.
	Improper reagent preparation	<ul style="list-style-type: none"> • Consult reagent preparation section for the correct dilutions of all reagents.
	Insufficient or prolonged incubation periods	<ul style="list-style-type: none"> • Consult the provided procedure for correct incubation time.
Deficient Standard Curve Fit	Non-optimal sample dilution	<ul style="list-style-type: none"> • Sandwich ELISA: If samples generate OD values higher than the highest standard point (P1), dilute samples further and repeat the assay. • Competitive ELISA: If samples generate OD values lower than the highest standard point (P1), dilute samples further and repeat the assay. • User should determine the optimal dilution factor for samples.
	Contamination of reagents	<ul style="list-style-type: none"> • A new tip must be used for each addition of different samples or reagents during the assay procedure.
	Contents of wells evaporate	<ul style="list-style-type: none"> • Verify that the sealing film is firmly in place before placing the assay in the incubator or at room temperature.
	Improper pipetting	<ul style="list-style-type: none"> • Pipette properly in a controlled and careful manner. • Check pipette calibration. • Check pipette for proper performance.

	Insufficient mixing of reagent dilutions	<ul style="list-style-type: none"> • Thoroughly agitate the lyophilized components after reconstitution. • Thoroughly mix dilutions.
--	------------------------------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------

References

- (1) Naot, D. *et al.* (2005) *Clinical Medicine & Research*. Vol 3, No. 2: 93-101
- (2) Brink, W. (October 2000) LE Magazine.
- (3) Yamauchi, K. *et al* (1993) *Infection and Immunity*. Vol 61, No 2, p.719-728
- (4) Conneely, O. M. (2001) *J.of the Am. Col. of Nutrition*. Vol. 20, No. 5, 389S-395S
- (5) Coremans IE. *et al.* (1993). *Adv Exp Med Biol* **336**:357-62. PMID: 8296635.
- (6) Loch H. *et al.* (1999) *Clin Exp Immunol*. **117**(3):568. doi: 10.1046/j.1365-2249.1999.01008.x. PMID: 1905360.

Version 1.1

Related Products

- EL2011-1 AssayMax Lactoferrin ELISA Kit (Plasma, Serum, Urine, Saliva, Milk, CSF, and Cell Culture samples)